

ZOLL® M Series® Defibrillator 12-Lead Report
2011-06-30 11:51:14


12-lead event 1 of 2

PATIENT NAME: _____
PATIENT ID: 201106301153
PATIENT AGE: 84
PATIENT SEX: Male

Vent Rate:	85	Normal sinus rhythm
P Duration:	112 ms	Low voltage QRS
PR Interval:	192 ms	Cannot rule out Anteroseptal infarct, possibly acute
QRS Duration:	94 ms	Lateral injury pattern
QT/QTc:	380/452 ms	** ** * * * Acute MI * * * * *
P-R-T Axis:	66 83 69	Abnormal ECG
		*** Unconfirmed ***

DEVICE ID: GOLDCROS000
RECORDED: 11:53:52 30 JUN 11

11:53:52 30 JUN 11

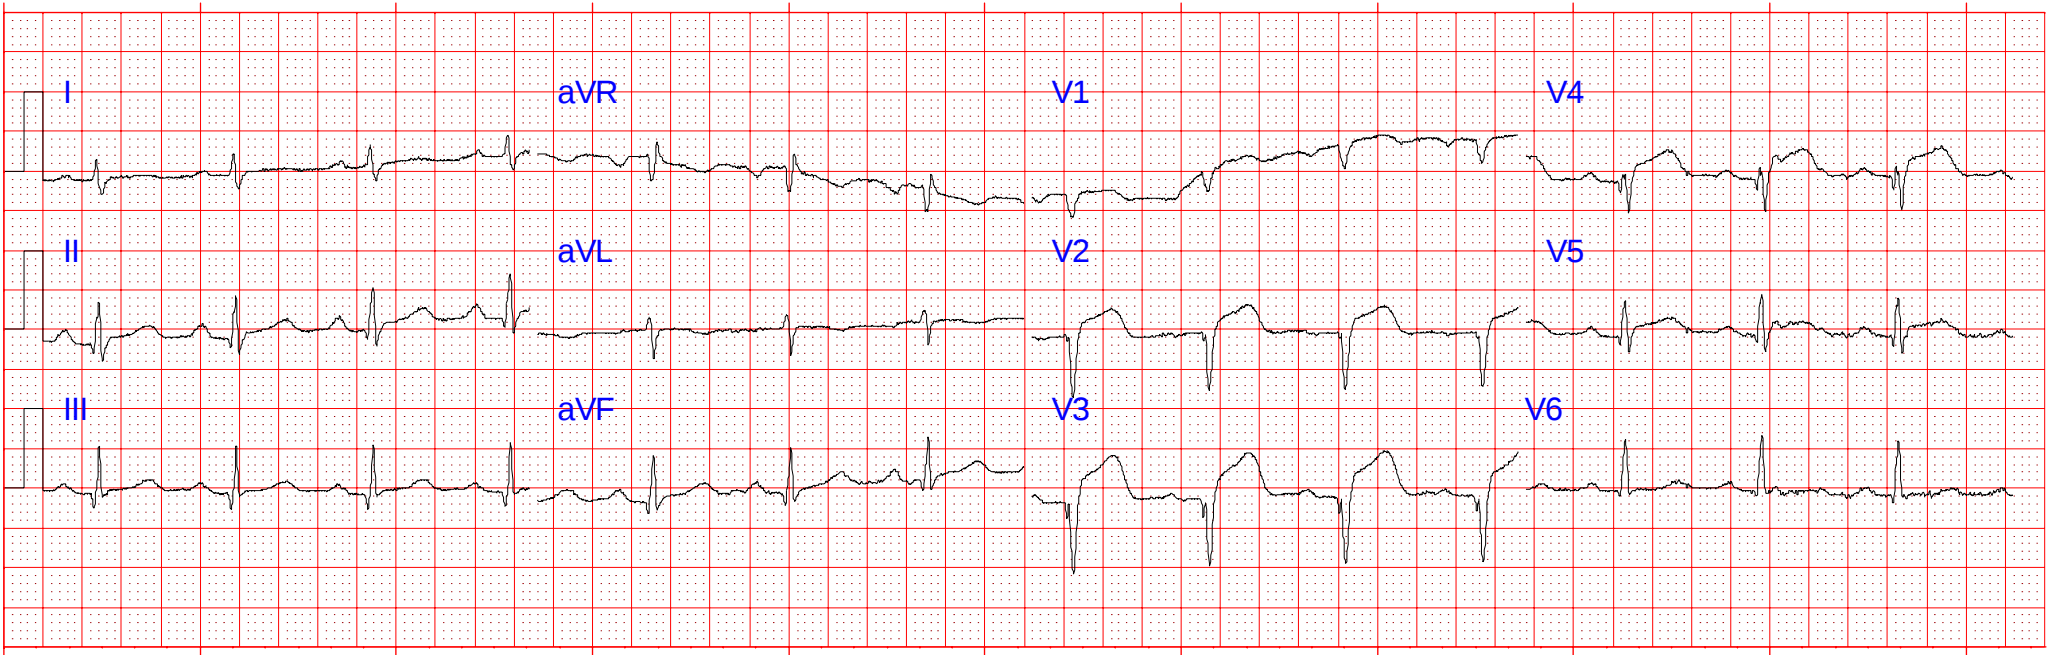

25 mm/s 10 mm/mV 0.05-150 Hz

Grid size is 0.20 s x 0.50 mV

	PA	PPA	QA	QD	RA	RD	SA	SD	RPA	RPD	SPA	STJ	STM	STE	TA	TPA
V1	-83	0	288	94	0	0	0	0	0	0	0	19	19	24	48	0
V2	14	-24	717	75	0	0	0	0	0	0	0	170	219	268	346	0
V3	68	0	864	73	0	0	0	0	0	0	0	283	361	439	590	0
V4	87	0	146	20	117	23	375	29	0	0	0	205	244	288	385	0
V5	87	0	87	17	458	33	195	22	0	0	0	131	151	175	229	0
V6	87	0	58	16	639	40	24	26	0	0	0	39	39	43	131	0
I	73	0	0	0	263	38	161	45	0	0	0	43	48	73	87	0
aVL	-24	0	0	0	141	31	312	63	0	0	0	4	0	4	-63	0
II	161	0	87	17	561	34	185	29	0	0	0	78	102	141	283	0
aVF	126	0	122	19	571	34	107	23	0	0	0	58	78	102	244	0
III	97	0	170	24	590	31	29	19	0	0	0	34	53	68	205	0
aVR	-117	0	0	0	24	13	297	36	170	31	0	-64	-79	-108	-185	0